

FIG. 1

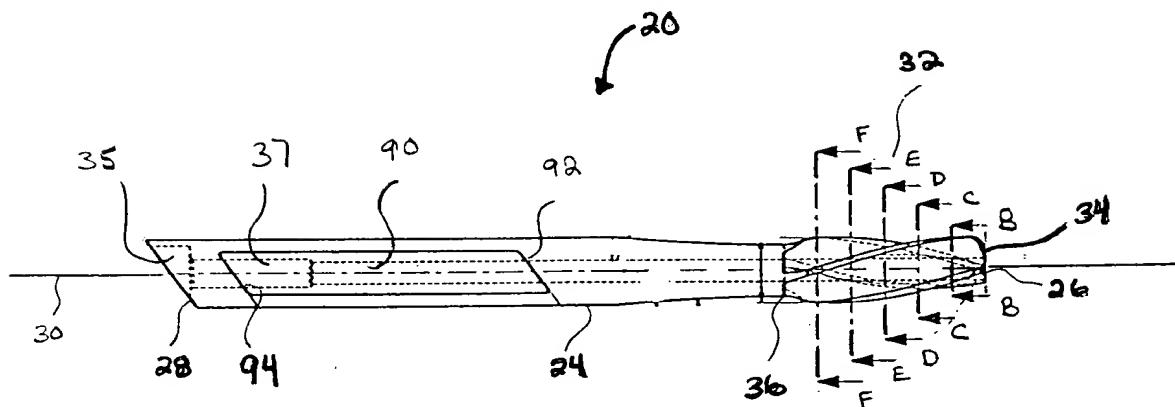


FIG. 2

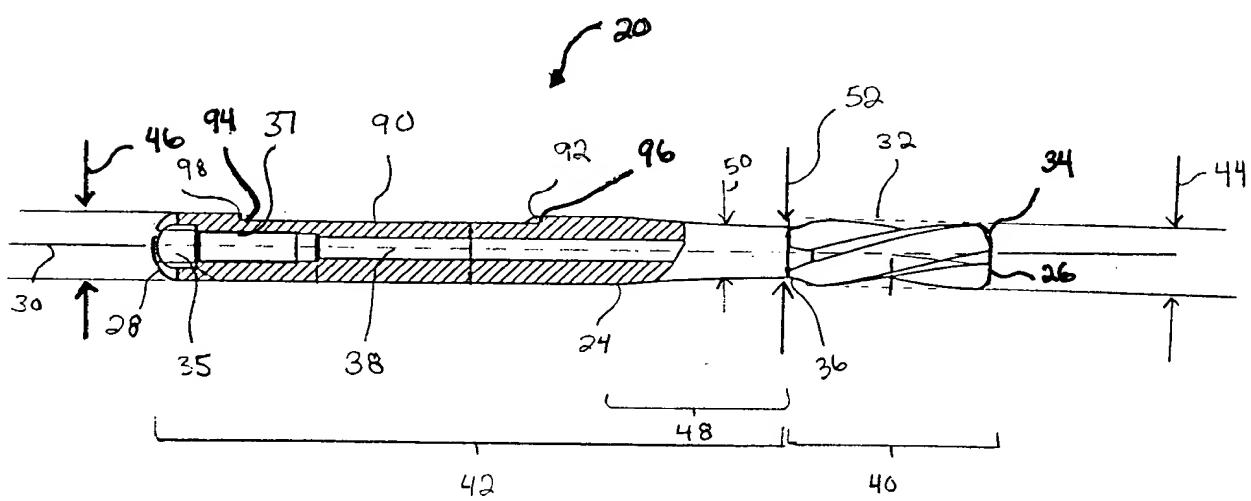


FIG. 3

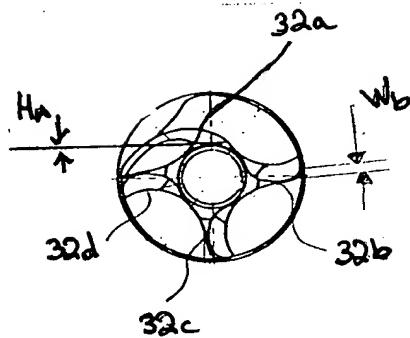


FIG. 4A

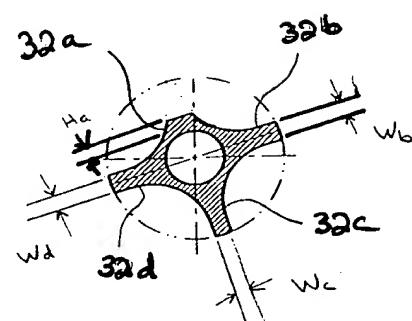


FIG. 4B

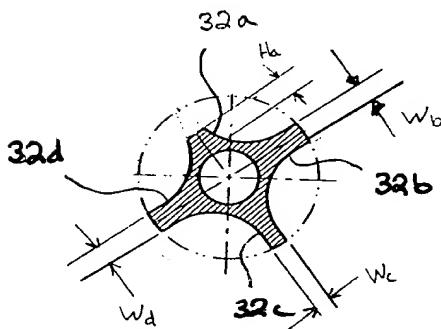


FIG. 4C

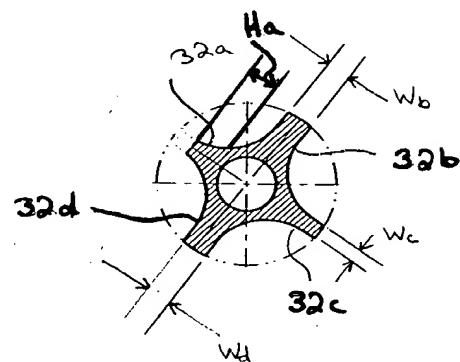


FIG. 4D

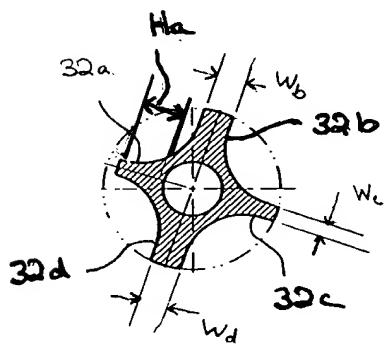


FIG. 4E

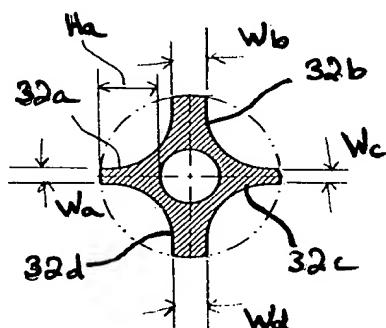


FIG. 4F

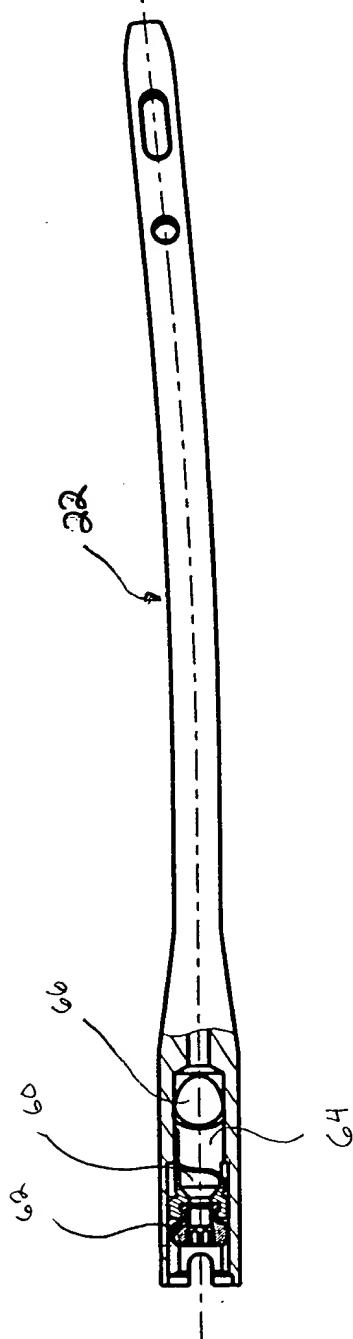


FIG. 5

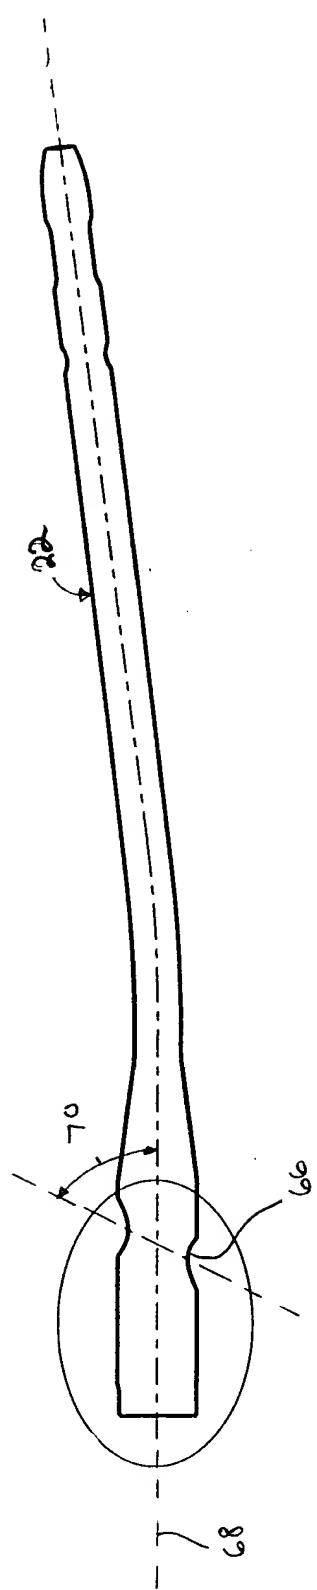


FIG. 6

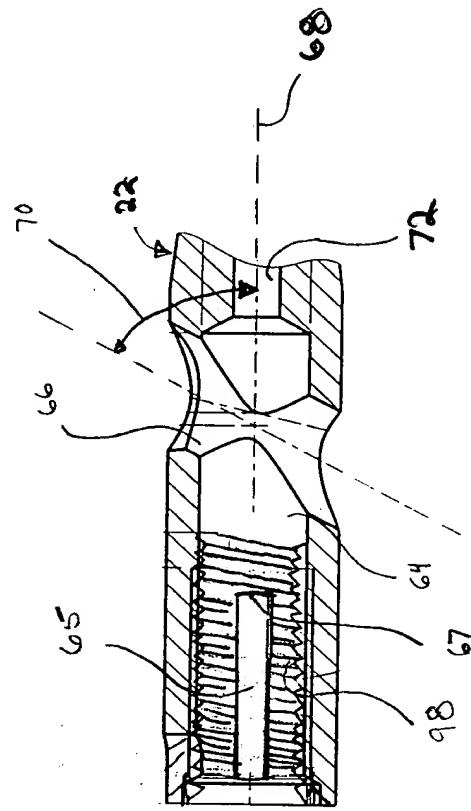
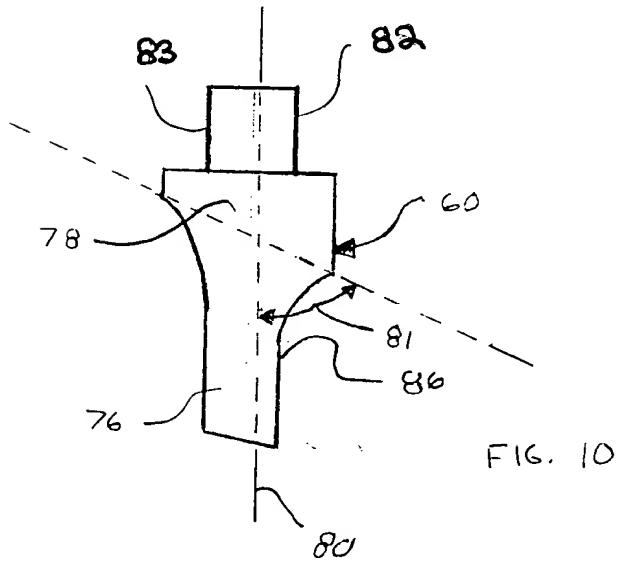
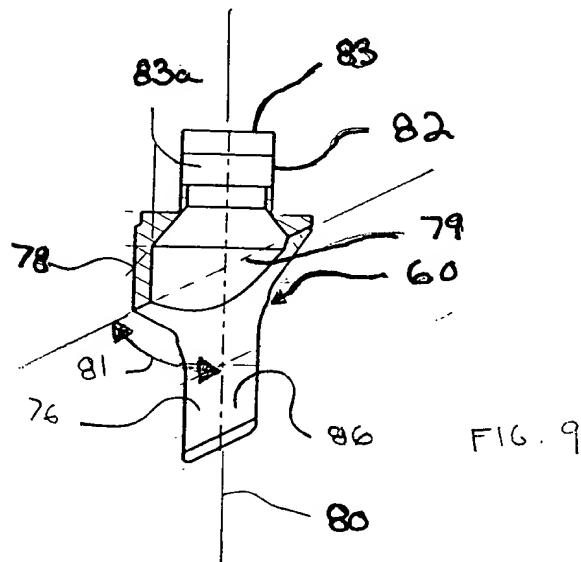
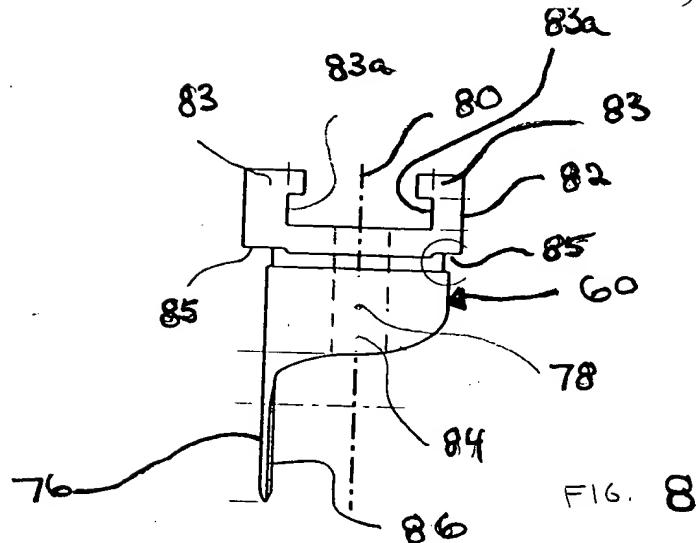


FIG. 7



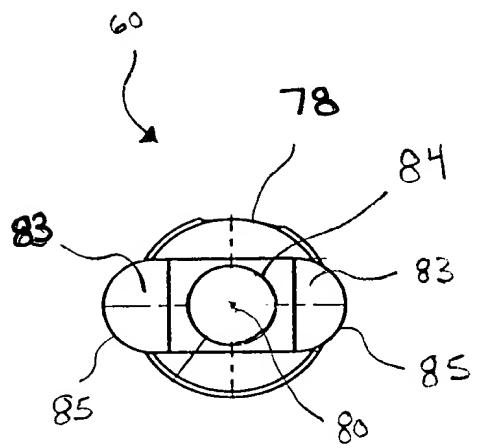


FIG. 11

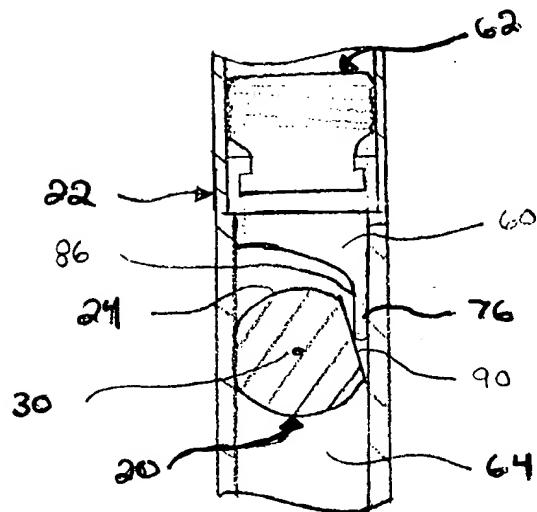


FIG. 12A

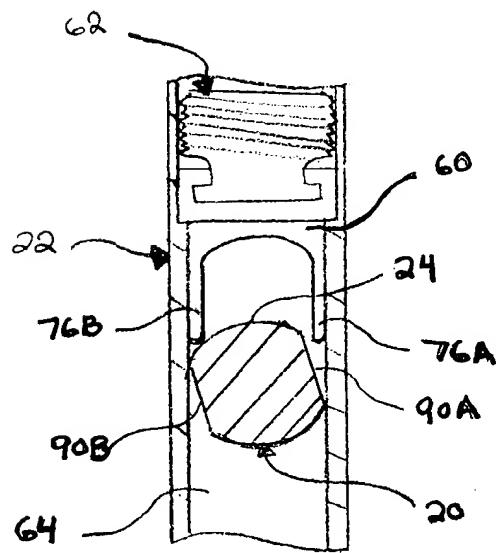


FIG. 12B

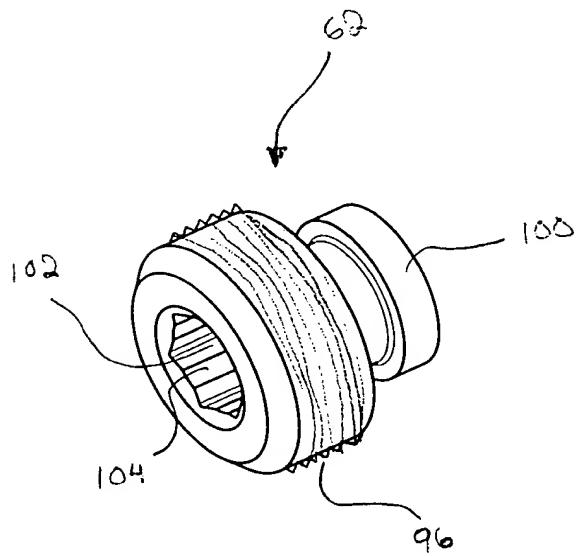


FIG. 13.

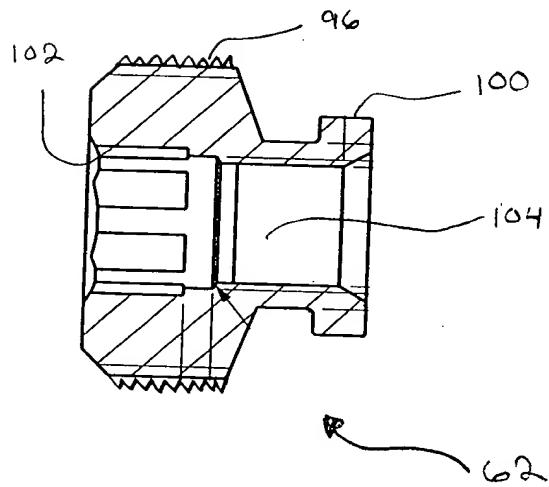
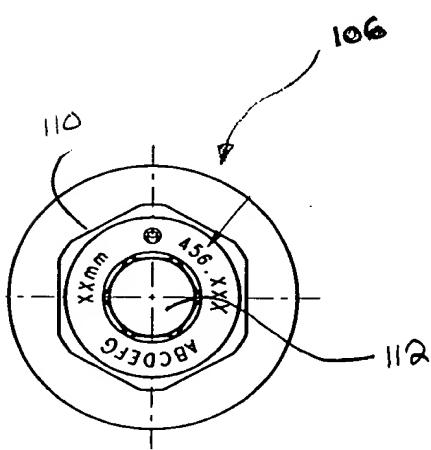
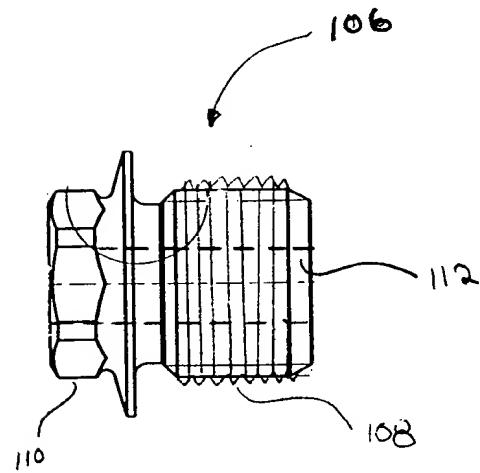


FIG. 14



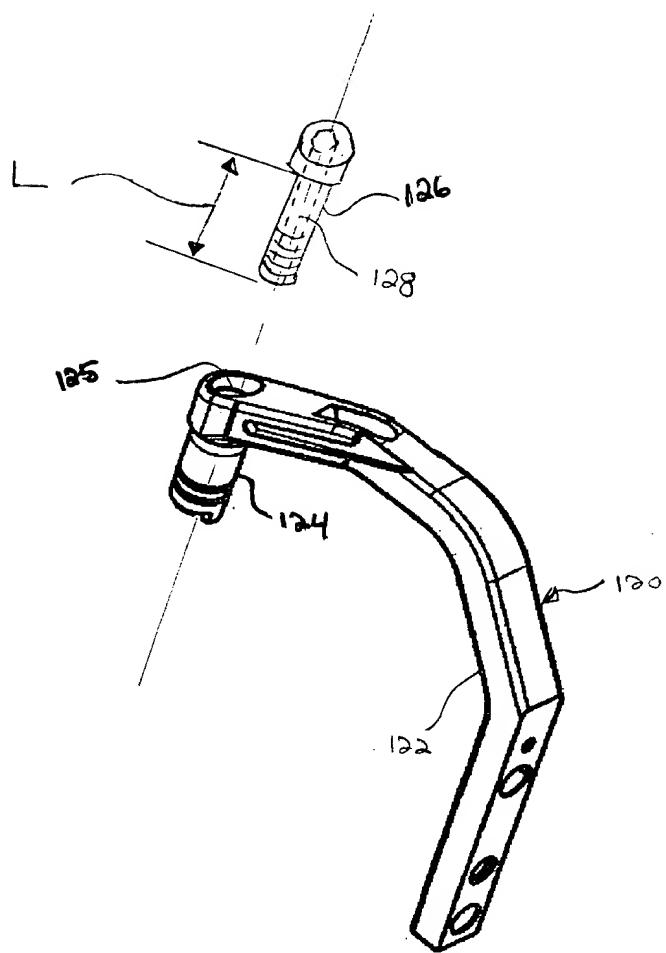


FIG. 17

New U.S. Application Of: Christoph
Andreas Roth; Filed: 10/17/01; For:
BONE FIXATION SYSTEM; Atty Dkt#
8932-266; Tel: 202-496-4400; Sht 12/12

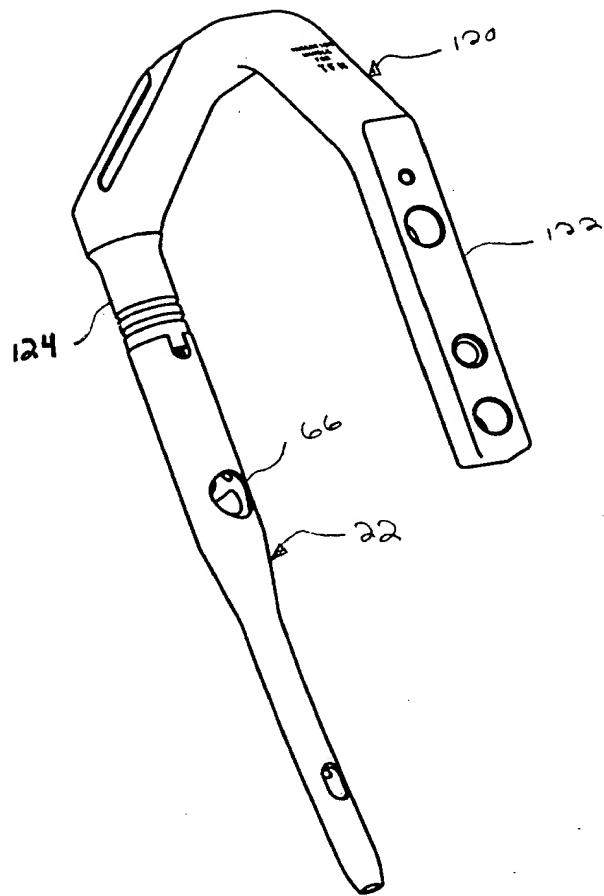


FIG. 18